

bioGenous™ Colorectal Cancer Organoid Selection Kit (Serum-free)

Catalog: K-2605

Product Description

bioGenous™ Colorectal Cancer Organoid Selection Kit is a serum-free culture medium specifically designed for the human colorectal cancer organoids. This kit supports the growth of patient-derived cancer organoids, which replicate the morphology, pathology, genetic, phenotypic, and behavioral traits of original tumours, while reducing the number of normal colorectal cells. This kit is a serum-free formulation that minimizes variability and ensures the reliable and reproducible culture of colorectal cancer organoids. bioGenous™ Colorectal Cancer Organoid Selection Kit is a powerful tool with significant potential for advancing medical research and precision medicine.

Product Information

Component	Catalog#	Volume	Storage& Stability
bioGenous™ Colorectal Cancer Organoid Selection Basal Medium	K-2605-A100/A500	100 mL/500 mL	2-8°C, 12 months
bioGenous™ Colorectal Cancer Organoid Selection Supplement B (50x)	K-2605-B100/B500	2 mL/10 mL	-20°C, avoid repeated freeze-thaw cycles, 12 months
bioGenous™ Colorectal Cancer Organoid Selection Supplement C (250x)	K-2605-C100/C500	0.4 mL/2 mL	-20°C, avoid repeated freeze-thaw cycles, 12 months

Materials & Reagents Required But Not Included

The following extended materials and reagents required for organoid maintenance can be purchased from www.biogenous.cn.

Manufacturer	Materials	Catalog#
bioGenous™	Primary Tissue Storage Solution (Serum-free)	K601005
bioGenous™	Cancer Organoid Selection Basal Medium (Serum-free)	B213152
bioGenous™	Tumour Tissue Digestion Solution	K601003
bioGenous™	Red Blood Cell Lysis Solution	E238010
bioGenous™	Anti-Adherence Rinsing Solution	E238002
bioGenous™	Organoid Cryopreservation Medium (Serum-free)	E238023
bioGenous™	Organoid Dissociation Solution	E238001
bioGenous™	Organoid Culture ECM (Reduced Growth Factor)	M315066
	Fetal Bovine Serum (FBS)	-
	DPBS (1x), liquid, contains no calcium or magnesium	-
	100 µm Cell Strainer	-

Safety Precautions

Always follow standard laboratory safety procedures when handling biological materials. Wear appropriate personal protective equipment (PPE), including gloves, lab coat, and eye protection. Dispose of waste materials according to local regulations.

For research use only, not for use in diagnostic procedures.


Preparation Before Use

Before initiating the protocol, ensure that all components and equipment are properly prepared:

1. Verify that all components are stored according to the guidelines provided in the manual. Avoid repeated freeze-thaw cycles for sensitive reagents. Thaw all necessary reagents according to the instructions. Keep on ice or at the recommended temperature until ready to use.
2. Ensure that all equipment, such as incubators, pipettes, and centrifuges, are calibrated and functioning correctly.

Preparation of Colorectal Cancer Organoid selection complete medium

Use a sterile technique to prepare the colorectal cancer organoid selection complete medium. The following example is for preparing a 10 mL complete medium. If preparing other volumes, adjust accordingly.

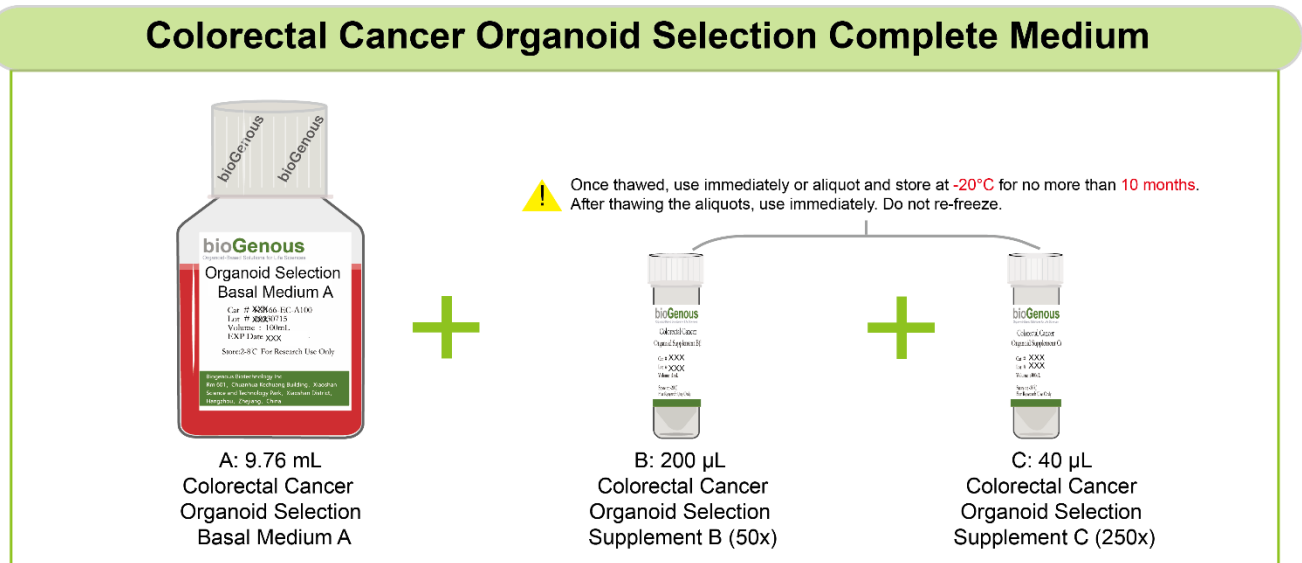

If not use immediately, store complete medium at **2-8°C** for no more than **2 weeks**. bioGenous™ Colorectal Cancer Organoid Selection Supplement B (50x) contains fungicide and antibiotics.

Colorectal Cancer Organoid Selection Complete Medium:

1. Thaw Colorectal Cancer Organoid Selection Supplement B (50x) and Colorectal Cancer Organoid Selection Supplement C (250x) on ice. Mix thoroughly.
2. Add 200 µL Colorectal Cancer Organoid Selection Supplement B (50x) and 40 µL Colorectal Cancer Organoid Selection Supplement C (250x) to 9.76 mL Colorectal Cancer Organoid Selection Basal Medium A. Mix thoroughly.

Protocol for Establishment of Patient-Derived Colorectal Cancer Organoids

Studies involving primary human tissue material must follow all relevant institutional and government regulations. Informed consent must be obtained from all subjects before the collection of the primary human tissue material.

Establishment of Organoids from Primary Tissue

1. Collect primary colorectal cancer biopsies in ice-cold Primary Tissue Storage Solution (K601005) using conical tubes. Keep tissue samples at 4°C until the start of the isolation.
2. Assess whether the obtained biopsies consist purely of tumour tissues. If fat or muscle tissues are present, remove these non-tumour components as much as possible using surgical scissors or scalpels and forceps under a dissection microscope. Otherwise, continue to the Step 3.
3. Rinse the tissue with Cancer Organoid Selection Basal Medium (B213152) or DPBS twice.
4. Mince the tissue into small fragments of 1-3 mm³ in a cell culture dish using surgical scissors or scalpels.
5. Digest the tissue fragments with 10 mL of Tumour Tissue Digestion Solution (K601003) in a 15 mL conical tube at 37°C, with variable incubation times ranging from 5 min to 30 min. Carefully monitor the digestion process, mixing the content of the tube every 5-10 min by shaking vigorously or pipetting the mixture up and down. The digestion process is complete when most of tissue fragments could pass through the 1 mL pipette tips.
6. Terminate tissue digestion by adding FBS to the tissue digestion mixture to a final concentration of 2% and filter using a 100 µm cell strainer.
7. Collect and centrifuge the filtered cells at 250 x g for 3 min at 4°C. In case of a visible red pellet, aspirate the supernatant and resuspend the pellet using 2 mL of Red Blood Cell Lysis Solution (E238010) to lyse the erythrocytes at room temperature for 1 min and centrifuge at 250 x g for 3 min at 4°C.
8. Aspirate the supernatant and resuspend the pellet in Cancer Organoid Selection Basal Medium, centrifuge at 250 x g for 3 min at 4°C. Repeat this step once more time.
9. Aspirate the supernatant and resuspend the pellet in bioGenous™ Organoid Culture ECM (M315066). The ECM should be kept on ice to prevent solidification. The amount of ECM used depends on the size of the pellet. Approximately 10,000 cells should be plated in 25 µL of ECM.

CRITICAL: Do not overly dilute the ECM (>70% (ECM vol/total vol)), as this may inhibit the proper formation of the solid droplets.

10. Seed the ECM containing cells at the bottom of 24-well cell culture plates in droplets of ~30 µL each around the center of the well.

CRITICAL: Once the organoids are resuspended in ECM, proceed as quickly as possible, as the ECM may solidify in the tube or pipette tip. Do not let the ECM touch the walls of well.

11. Prepare the required amount of colorectal cancer organoid selection complete medium.
12. Once the ECM droplets have solidified (15-25 min) and carefully add 500 µL organoid selection complete medium to each well.

CRITICAL: Do not add the medium directly on top of the ECM droplets, as this might disrupt the droplets.

13. Place the culture plate in a humidified incubator at 37°C and 5% (vol/vol) CO₂.
14. Change the medium every 3-4 days by carefully aspirating the medium from the wells and replacing it with a fresh, pre-warmed organoid selection complete medium.
15. Closely monitor the organoid formation. Ideally, patient-derived colorectal cancer organoids should be passaged for the first time between 10 and 14 days after the initial seeding. Typical morphologies of successfully cultured patient-derived human colorectal cancer organoids are shown in Figure 1.

Splitting and Passaging of Organoids

1. Pipette up and down to disrupt the ECM and transfer the organoid suspension to a 1.5 mL tube. Continue pipetting up and down to create pressure to help remove the ECM.
2. Centrifuge the tube at 250 x g for 3 min at room temperature.
3. Aspirate the supernatant and split the organoids using either Organoid Dissociation Solution (E238001) or by mechanical disruption.

Organoid dissociation solution-based cell dissociation: Resuspend the pellet in 0.2 mL of Organoid Dissociation Solution, pipette up and down and incubate at 37°C until the organoids are released from the ECM. Pipette up and down with a filter tip for ≥8 times every 2 min to aid in the disruption of the organoids. Closely monitor the digestion to keep the incubation time in the Organoid Dissociation Solution to a minimum.

Mechanical disruption-based cell dissociation: Resuspend the pellet in 1.5 mL of Cancer Organoid Selection Basal Medium. Carefully pipette the organoid suspension up and down 30 times by pipetting against the bottom of the tube to create pressure, which will aid organoid disruption.

CRITICAL: Do not dissociate in Organoid Dissociation Solution for >7 min, as this may result in poor organoid outgrowth or even loss of the culture. As a rule of thumb, digestion is complete if a mixture of small lumps of cells (consisting of 10-50 cells) can be observed.

4. After shearing is complete, wash once by adding 1 mL Cancer Organoid Selection Basal Medium and centrifuge at 250 x g for 3 min at room temperature.
5. Aspirate the supernatant and resuspend the organoid pellet in 70% (vol/vol) ECM, and plate organoids in droplets at the bottom of a culture plate. After seeding, transfer the culture plates to a humidified incubator at 37°C and 5% (vol/vol) CO₂ for 15-25 min.
6. Pre-warm the colorectal cancer organoid selection complete medium at 37°C.
7. After the ECM droplets have solidified (15-25 min), carefully pipette the pre-warmed medium into the wells.
8. Place the culture plates in a humidified incubator at 37°C and 5% (vol/vol) CO₂ until the organoids are needed for further experiments.

Applications

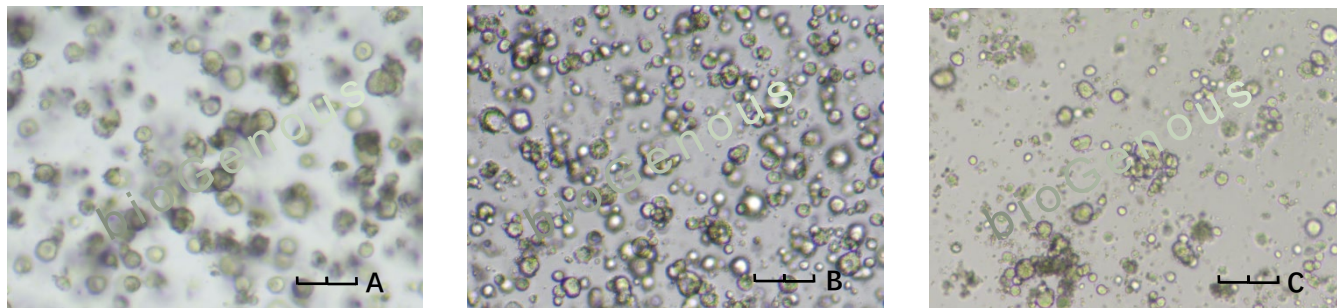


Figure 1. Morphological examples of successfully cultured colorectal cancer organoids derived from different patients at day 7 (A), day 7 (B) and day 7(C), respectively. Scale bar: 200 μ m.

Quality Control

All components are negative for bacterial and fungal contamination. Certificate of authenticity (COAs) for all other products are available upon request.

Safety information

Read the Safety Data Sheets (SDSs) and follow the manufacture's instruction.

Disclaimer

To the fullest extent permitted by applicable law, bioGenous BIOTECH, Inc. and/or its affiliates shall not be liable for any special, incidental, indirect, punitive, multiple, or consequential damages arising from or related to this document or your use thereof.

Contact and Support

For questions, suggestions, and technical supports, please contact us at E-mail: info@biogenous.cn.

Last updated on 30th August, 2025